

High Voltage Differential Probes

DP6000D Series

DP6070D 700Vpk/500MHz

DP6150D 1500Vpk/500MHz

DP6280D 2800Vpk/500MHz

DP6700D 7000Vpk/500MHz



ShenZhen ZhiYong Electronics Co., Ltd



Introduction

First of all, thank you for purchasing our products, this instruction manual is the description about the function, usage, operation attention points, etc. Before use, please read the instructions carefully and use correctly.

Manual annotation will use the following symbols to distinguish.



This symbol means it is harmful to the machine and human body; you must strictly follow the instruction manual to operate.



In the case of wrong operation, the user risk injury. The content under this mark records the relevant matters needing attention to avoid such dangers.



The user may suffer minor injuries and material damage with the wrong operation. To avoid such situation, the matters under this mark need



This symbolizes important note about how to use the machine.

To the safely use the machine, you must abide by the following safety precautions strictly. The violation against the manual is likely to damage the protective function of the machine. In addition, the company is not responsible for any safety problem caused by the violation of matters needing attention in operation.



- Please be careful to the danger of electric shock and pay attention to highest input voltage.
- Do not operate in wet or combustible conditions.
- Make sure the circuit under test is turned off before access it to the probe.
- Turn off the circuit after the measurement, and then remove the probe.
- When BNC lines are connected to the oscilloscope or other devices, ensure the BNC terminal is well grounded.
- Please check the probe skin. If there is any breakage, stop using it immediately.
- Select the product standard adapter power supply.

DP6000D Series Brief Description

Modal	Maximum Input Differential Voltage	Bandwidth	Attenuation
DP6070D	700V	500MHz	20X/200X
DP6150D	1500V	500MHz	100X/1000X
DP6280D	2800V	500MHz	200X/2000X
DP6700D	7000V	500MHz	200X/2000X



Contents

Introduction1
DP6000D Series Brief Description
Summary3
Application
Products and Accessories
Main part of probe4
Accessories5
Specifications7
Machinery specification
Environment Specifications8
Operating steps8
Test mode(Offset Settings)8
Precautions For Use
Performance Verification
Installation11
DC accuracy11
Rise time
DC common mode rejection ratio (CMRR)
Test records form
Maintenance
Warranty13
Packing List14



1. Summary

- DP6000D Series High Voltage Differential Probe is designed with floating measurement function, with a maximum bandwidth up to 500MHz that can fulfill the need of most measuring system.
- DP6000D Series provides a wide measuring range for selection, and its differential measurement voltage range can meet the requirement of most measurement circuit.
- The users can enter the test mode to adjust the offset voltage of the probe and realize zero set.
- DP6000D Series provides a 5MHz bandwidth limit function. 5MHz frequency bandwidth can meet the
 measurement of the switching frequency of most FETs in switching power supplies, and can filter out
 higher frequency noise and interference.
- DP6000D Series has sound & light alarming function, and users can turn it off manually if needed.
- DP6000D Series is powered by USB connector, and it contains standard BNC output connector that can adapt oscilloscope of any brand. In which, requires oscilloscope input impedance set to 50 Ω (recommended) or connecting a through type 50 Ω load while setting the input impedance to 1M Ω .
- The probe has good CMRR, with high input impedance and low capacitance at the input end, which can accurately and quickly measure differential voltage signals. It can be widely used in the research and development, debugging, or maintenance of switching power supplies, frequency converters, electronic ballasts, variable frequency household appliances, and other electrical power devices.

2. Application

- Floating voltage measurement
- Inverter
- Switch Power Supply
- Welding, plating power supply
- Induction heating, electromagnetic oven
- Motor driver design
- Electronic ballast design
- CRT display design
- Inverting, UPS power supply
- Inverter appliance
- Power conversion and related design
- Experiment of electrical engineering
- ♦ Low voltage test
- ♦ Power electronics and power transmission experiment, etc




3. Products and Accessories

■ Main part of probe

As DP6150D for example, different voltage, range, bandwidth would be in different product.



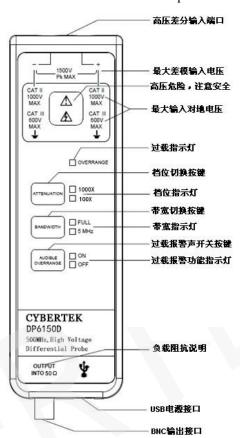


Detailed instructions

- ♦ Integral input leads: The integral input leads extend 28cm from the probe body. Connect the leads directly to your circuit, or use the extender leads and other accessories.
- ♦ ATTENUATION: Different attenuation indicates different ranges, such as DP6150D: 1000X, indicate the maximum test voltage is 1500V. 100X presents maximum test voltage is 150V. DP6700D: 2000X shows maximum test voltage is 7000V. 200X indicate maximum test voltage is 700V; oscilloscope attenuation factor should be set accordingly based on the probe attenuation selection.
- ♦ BANDWIDTH: The series products have bandwidth selection function; the default is full bandwidth (FULL) of the product. When testing low frequency signal, you can choose 5MHz bandwidth limit to prevent being interfered by high frequency signal.
- ♦ AUDIBLE OVERRANGE: When test range exceeds probe range, audible and visual alarm will start; the function is to control buzzer alarm on or off, ON is to open audible alarm and OFF closes the alarm.
- \diamond Output connector: Standard BNC output connectors, can be connected to any oscilloscope of any brand. requires the input impedance of the oscilloscope set to 50 Ω (recommended), or connect with standard through type 50 Ω load and set the input impedance to 1M Ω .
- ♦ Power interface: Standard USB type B interface, supply power with standard USB adapter, can be supplied by oscilloscope, easy to use, also can be supplied by portable power source, convenient for outdoor test
- → Factory Setting: The default factory setting is high attenuation ratio, FULL bandwidth, audible alarm is on. The product has automatic memory, automatically save the state before power off.



■ Accessories Description

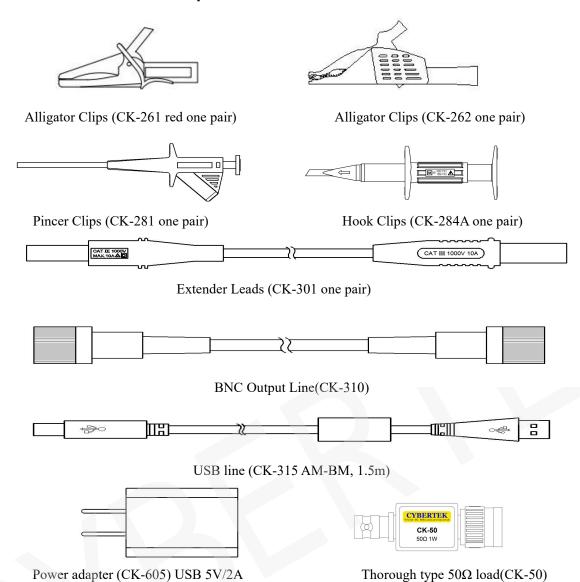

Product standard accessories description:

Modal	DP6070D	DP6150D	DP6280D	DP6700D	
Alligator Clips(CK-261)	CATIII 1000V				
Anigator Chps(CK-201)		CATIV 600V			
Alligator Clips(CK-262)				CATIII 1000V	
Anigator Crips(CK-202)				CATIV 600V	
Pincer Clips(CK-281)	CATIII 1000V				
Hook Clips(CK-284A)	CATIII 1000V				
Extender Leads (CK-301)	CATIII 1000V				
BNC Output Line((CK-310)	Double-ended BNC connector coaxial line 1m				
USB Line (CK-315)	1.5m				
Power Adapter (CK-605)	USB 5V/2A				
Thorough type 50Ω load(CK-50)		50Ω	1W		

NOTE: The above "--" refers to non-standard accessory of this model.



4. Electric Specification

Model			DP6070D DP6150D DP6280D D			DP6	700D			
Bandwidth(-3	dB)	500MHz								
Rise time		≤700ps								
Accuracy			±2%							
Range selection (Attenuation r		202	X/200X	100X	/1000X	200	X/2000X	200X/	200X/2000X	
Maximum dif voltage(DC +		20X 200X	$\pm 70V$ $\pm 700V$	100X 1000X	±150V ±1500V	200X 2000X	±280V ±2800V	200X 2000X	$\pm 700V$ $\pm 7000V$	
Common mod + Peak AC)	le voltage(DC	<u>+</u>	700V		500V	土	2800V	±7	000V	
Maximum diff VS frequency	ferential mode curve		erence gure 1	Fig	ure 2	Figure	3	Figu	ire 4	
Maximum inp voltage-to-ear			V CATII V CATI		CATIII / CATII		CATIII V CATII		CATIII / CATI	
Input	Single-ende d to ground	2.	5ΜΩ	5	ΜΩ	Ę	5Μ Ω	20	MΩ	
impedance	Between inputs Single-ende	:	5ΜΩ	10)ΜΩ	1	OM Ω	40	MΩ	
Input capacitance	d to ground Between		<4pF		54pF		<4pF	<5pF		
сиристипсс	inputs		<2pF		2pF		<2pF	<2.5pF		
CMRR	DC		>80dB		>80dB >80dB		>80dB			
CMKK	100kHz		-60dB	>60dB >50dB		>60dB >50dB		>60dB >50dB		
	1MHz	20X	>50dB <85mV	100X	<200mV	200X	<240mV	200X	<625mV	
Noise(Vrms)		200X	<130mV	100X	<420mV	200X	<660mV	200X 2000X	<1V	
Differential or detection leve	_	20X	≥70V ≥700V	100X	≥150V	200X	≥280V	200X	≥700V	
	Probe	200X	= 100V	1000X	≥1500V	2000X About 6ns	≥2800V	2000X	≥7000V	
Propagation time	BNC Line(1m)				A	About 5ns				
Bandwidth lir (5MHz)					≥-3	dB@5MF	Iz			
Overload indi (red light)	cator					Yes				
Overload alar	m	Yes(Can shut up manually)								
Automatic sav	ve	Yes								
Offset setting function				Yes (S	et in test m	node)				
Terminate loa	Terminate load 50 Ω									
Power supply					USB 5	5V/2A ada	pter			
Safety standard EN61010-1: 2010										
EMC standard	d	EN61326-1:2013 EN61000-3-2:2006+A1:2009+A2:2009 EN61000-3-3:2013				06+A1:20	09+A2:2009	EN61000-	3-3:2013	



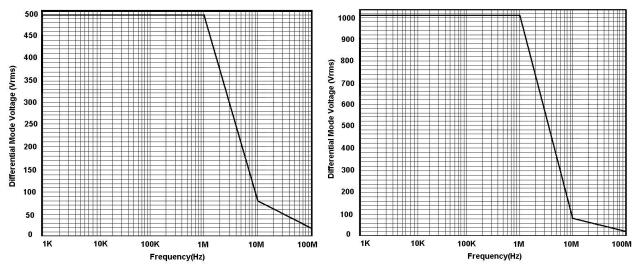


Figure 1:DP6070D Differential Mode Voltage VS Frequency

Figure 2:DP6150D Differential Mode Voltage VS Frequency

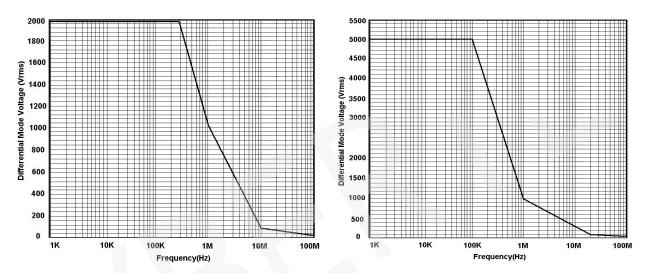


Figure 3:DP6280D Differential Mode Voltage VS Frequency Figure 4:DP6700D Differential Mode Voltage VS Frequency

5. Mechanical Specification

Model	Parameters
Input leads	Approx 28cm
Extender leads(CK-301)	Approx 1m
BNC Output Line(CK-310)	Approx 1m
Alligator clips CK-261	Approx 85*40*17mm
Alligator clips CK-262	Approx 106*43*16mm
Pincer clips CK-281	Approx 152*50*13mm
Hook clips CK-284A	Approx 121*37*20mm
Probe dimensions	Approx 195*58*25mm
Probe weight	Approx 250g



6. Environmental Characteristics


Model	Parameters
Operating temperature	0℃~50℃
Storage temperature	-30°C ~70°C
Operating humidity	≤85%RH
Storage humidity	≤90%RH
Operating altitude	3000m
Storage altitude	12000m

7. Operating steps


- ♦ You should estimate the tested voltage amplitude before testing. Please do not use if exceeds the voltage range, or the probe could be damaged.
- Connect the input lead and output lead to the probe, and then connect the probe to oscilloscope or other instruments.
- ♦ Connect the power adapter to voltage probe, the power indicator light turns on green. Please select proper range based on the tested voltage; when the tested voltage exceeds range, the overload indicator light is on with alarming sound, which can be manually turned off.
- ♦ Please set proper attenuation rate for the oscilloscope or other instruments according to the probe range; and adjust the oscilloscope sensitivity based on the tested voltage.
- ♦ Connect the probe clips based on needs, start after connecting to the circuits to be tested. When testing, the probe body should keep away from high voltage pulse circuits to reduce interference to the probe.
- ♦ Turn off the probe power after the testing is completed, first disconnect the two inputs from the tested points, and then unplug the BNC plug from the oscilloscope.


8. Test Mode (Offset Setting)

User may enter the test mode to adjust offset if the output zero drift. The adjustment method is as follows:



→ Turn power on to start, you will be in test mode while the overload indicator light is on, then release the two keys.






After the above step, press key to exit the test mode, offset adjustment is completed and the overload indicator light off, entering into normal operation mode.




9. Safety Notices:




Please try to wind the input leads when testing, which is better for eliminating noise, to improve the ability of high frequency response.
Please view below for the winding method:

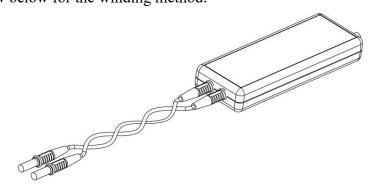

♦ It is better not to extend input lead when testing; otherwise it may introduce more noise. If extra extension lead is necessary, please ensure the extension leads are at same length, and the input frequency is under 5MHz, errors may exist if exceeds 5MHz output.

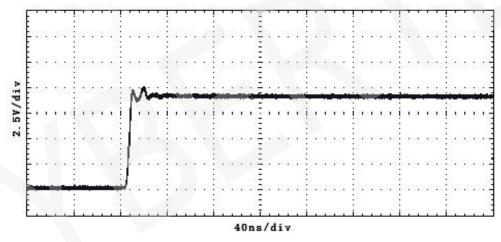

Without extender leads

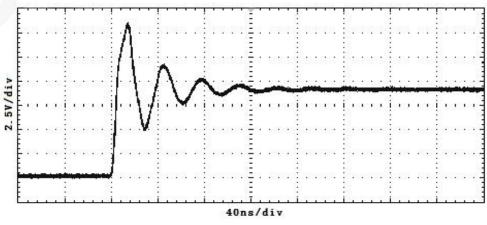

With extender leads



10. Performance Verification

The below operation is for performance verification of the electric specification, requirement for test equipment is shown below:

Equipment	Minimum Requirements	Usages
Oscilloscope	Bandwidth≥500MHZ; Accuracy ≤ 1.5%, e.g. Tektronix MSO/DSO4000	Displays probe output
Standard signal generator; calibrator	Amplitude accuracy≤0.75%; rise time≤700ps e.g.: FLUKE/WAVETEK 9100	Test bandwidth; AC accuracy; common mode rejection ration
Digital multimeter	Accuracy of not less than 6 and a half e.g.: KEITHLEY 2000	Test the DC accuracy
Insulation pincer clips	Supplied in the accessories	Testing clips
BNC adapter 1	BNC-male-to-female-dual show as Figure 1	Test adapter
BNC adapter 2	BNC-male-to-dual binding post show as Figure 2	Test adapter
BNC adapter 3	BNC-female-to-dual binding post show as Figure 3	Test adapter
Load terminal	BNC-male-to 50Ωload show as Figure 4	Signal source load




Figure 1 BNC-male-to-female-dual




Figure 2 BNC-female-to-dual binding post




Figure 3 BNC-male-to-dual binding post



Figure 4 BNC-male-to 50Ω load



10.1 Setup

- ♦ Connect power adapter to voltage probe, which turns on green light, to ensure accuracy, test the probe index after 20 minutes.
- ♦ Uncover the red black plastic cover of the BNC-male-to-dual binding post.

10.2 DC Accuracy

- Connect the probe output to the BNC-female-to-dual binding post; plug the two input terminals of the digital multimeter into the binding post hole.
- ♦ Connect the probe input to insulation pincer clips, and then connect the calibrator output and the generator close, connect the red clip to the positive pole, black clip to negative pole.
- ♦ Set the probe attenuation factor in the first gear.
- ♦ Follow the chart below to set output values for the signal source.
- ♦ Enable the signal output, observe and record the output voltage for the attenuation.
- ♦ Close the signal source output.
- ♦ Switch the probe attenuation factor to the second gear.
- \diamond Repeat step 4~6, and calculate whether is within the accuracy ranges.

Model	Attenuation Rate	Signal source output voltage	Probe expected output voltage	Probe practical output voltage
DD6070D	20X	2V	100mV±2mV	
DP6070D	200X	20V	100mV±2mV	
DP6150D	100X	10V	100mV±2mV	
	1000X	100V	100mV±2mV	
DD6280D	200X	20V	100mV±2mV	
DP6280D	2000X	200V	100mV±2mV	
DP6700D	200X	20V	100mV±2mV	
	2000X	200V	100mV±2mV	

10.3 Rise Time

- \diamond Configure the fast rise output of the generator for a 50 Ω load. Attach a 50 Ω terminator to the generator fast-rise output and attach the modified BNC adapter to the terminator. Attach the differential probe input leads (without attachment accessories) by sliding the banana plug of the leads onto the binding posts metal sleeves on the modified BNC adapter.
- ♦ Connect the probe output to the oscilloscope, set attenuation factor in the first gear.
- → Refer to the below stable to set standard signal generator.
- ♦ Enable signal source output and record the rise time.
- ♦ Close signal source output.
- ♦ Switch the probe attenuation factor to the second gear.
- \diamond Repeat step 3~5, and calculate whether is in the range.



Model	Attenuation Rate	Signal source voltage, frequency setting	Expected probe rise time	Rising time
DP6070D	20X			
טו טטוטט	200X			
DP6150D	100X	20Vp-р 500МНz		
DE0190D -	1000X		~700	
DP6280D —	200X		≤700ps	
	2000X			
	200X			
DP6700D	2000X			

10.4 DC Common Mode Rejection Ration(CMRR)

- ♦ Set DP6000D series probes at low attenuation ration, respectively (20X, 100X, 200X).
- ♦ Set 500V DC voltage for signal source, now the voltage output shut up.
- ♦ Connect the two probe inputs to 500V voltage.
- ♦ Connects the probe output to BNC-female- to- dual binding post (as shown in Figure 3), and plug into the two inputs of the digital multimeter.
- ♦ Enable signal source output, respectively record voltage output values; check with the following chart to calculate whether is within the ranges.
- ♦ Close the calibrator after completion of the test.

Model	Attenuation Rate	Probe expected output voltage	Probe practical output voltage
DP6070D	20X	≤1mV	
DP6150D	100X	≤1mV	
DP6280D	200X	≤1mV	
DP6700D	200X	≤1mV	

Note: High voltage 500 V is used during the testing, please pay attention to personal safety; to reduce voltage fluctuation, be sure to make the calibrator output 500 V high voltages after the completion of all connections.



10.5 Testing Record Form

Testing Record Form						
Product serial NO:			Test temperature:			
Testing date:			Test Humidity:			
Test model:			Lower limit	Test result	Upper limit	
	DP6070D	20X	98mV		102mV	
	עטיזטטאע	200X	98mV		102mV	
	DP6150D	100X	98mV		102mV	
DC	עטפוסאע	1000X	98mV		102mV	
DC accuracy	DDGQQD	200X	98mV		102mV	
	DP6280D	2000X	98mV		102mV	
	DP6700D	200X	98mV		102mV	
		2000X	98mV		102mV	
	DP6070D	20X			700ps	
		200X			700ps	
	DP6150D	100X			700ps	
D: 4:		1000X			700ps	
Rise time	DD COOOD	200X			700ps	
	DP6280D	2000X			700ps	
	DD2700D	200X			700ps	
	DP6700D	2000X			700ps	
	DP6070D	20X			1 mV	
DC common mode rejection ratio	DP6150D	100X			1 mV	
	DP6280D	200X			1 mV	
	DP6700D	200X			1 mV	

11. Care and Maintenance

- → Keep the probe clean and dry.
 - ♦ Please wipe with soft dry cloth when clean needed, must not use chemicals to clean.
 - ♦ Please put the probe in the package provided, and put it in cool, clean and dry places.
 - ♦ Please put the probe in the package provided to prevent shock.
 - ♦ Do not forcefully pull the input and output lead to prevent bending, twisted and folding.

12. Warranty

Please refer to the warranty instruction.



13. Packaging

Package				
Items	DP6070D	DP6150D	DP6280D	DP6700D
Voltage probe body	1 unit	1 unit	1 unit	1 unit
USB 5V/2A Adapter(CK-605)	1 unit	1 unit	1 unit	1 unit
Alligator clips (CK-261)	1 pair	1 pair	1 pair	
Alligator clips (CK-262)				1 unit
Insulation pincer clips (CK-281)	1 pair	1 pair	1 pair	1 pair
Hook clips (CK-284A)	1 pair	1 pair	1 pair	1 pair
Extension cord (CK-301)	1 pair	1 pair	1 pair	1 pair
Output lead(CK-310)	1 pcs	1 pcs	1 pcs	1 pcs
USB connecting line (AM-BM, 1.5m)	1 pcs	1 pcs	1 pcs	1 pcs
User manual	1 book	1 book	1 book	1 book
Warranty card	1 unit	1 unit	1 unit	1 unit
Testing report	1 pcs	1 pcs	1 pcs	1 pcs
Thorough type 50Ω load(CK-50)	1 unit	1 unit	1 unit	1 unit

NOTE: The above "--" refers to non-standard accessory of this model



CYBERTEK

SHENZHEN ZHIYONG ELECTRONICS CO., LTD.

Addr: Room A1702, Building 4, TianAn Cyber Park, HuangGe Road, LongGang

District, ShenZhen City, China

Tel: (86) 400 852 0005

(86 755) 86628000

Q Q: 400 852 0005

Email: cybertek@cybertek.cn © Zhiyong Electronics, 2024

Url: http://www.cybertek.cn Published in China, Jan. 1, 2024